

Bode 100 - Application Note

Impedance Measurement of a Three-Phase Motor



By Hugo Huaman

© 2025 by OMICRON Lab – V1.0

Visit www.omicron-lab.com for more information.

Contact support@omicron-lab.com for technical support.

Table of Contents

1	Executive Summary	3
2	Measurement Tasks	3
3	Measurement Setup	4
	3.1 Device Under Test (DUT).....	5
	3.2 DUT Connection.....	5
	3.3 Bode Analyzer Suite (BAS) Setup.....	6
	3.4 Calibration	7
4	Results	8
5	Conclusion	10

Note: Basic procedures such as setting-up, adjusting and calibrating the Bode 100 are described in the Bode 100 user manual available at:

<https://www.omicron-lab.com/downloads/vector-network-analysis/bode-100/>

Note: All measurements in this application note have been performed using the Bode Analyzer Suite V3.51 Use this version or a newer version to perform the measurements shown in this document. You can download the latest version at

<https://www.omicron-lab.com/downloads/vector-network-analysis/bode-100/>



1 Executive Summary

Understanding the impedance of a three-phase motor can help ensuring optimal performance, efficiency, and safety. Measuring the impedance of the winding can be useful to identify issues such as short circuits, insulation failures and winding damage. When operating a motor via variable frequency inverters, the switching waveforms generate high-frequency signals. The impedance of the winding varies strongly over frequency, impacting the current flow caused by these voltages.

Balanced winding impedance ensures equal magnetic field distribution enhancing overall performance. The capacitance between neutral and motor housing is a property of the insulation. Maintaining a low capacitance reduces ground leakage currents which can impact EMI behavior.

The scope of this application note is to provide a reliable setup for the impedance measurement with the Bode 100. This application note details the connection setup and the device setting of the Bode 100 necessary to perform the impedance measurement.

2 Measurement Tasks

The Device Under Test (DUT) for the measurement is a simple asynchronous three-phase motor. The One-Port method was selected since its impedance range is ideal for typical motor winding and housing capacitance impedance. In this application note, we measure the winding-impedance between phase and neutral as shown in Figure 1 a) and the insulation-impedance between the neutral point and housing as shown in Figure 1 b).

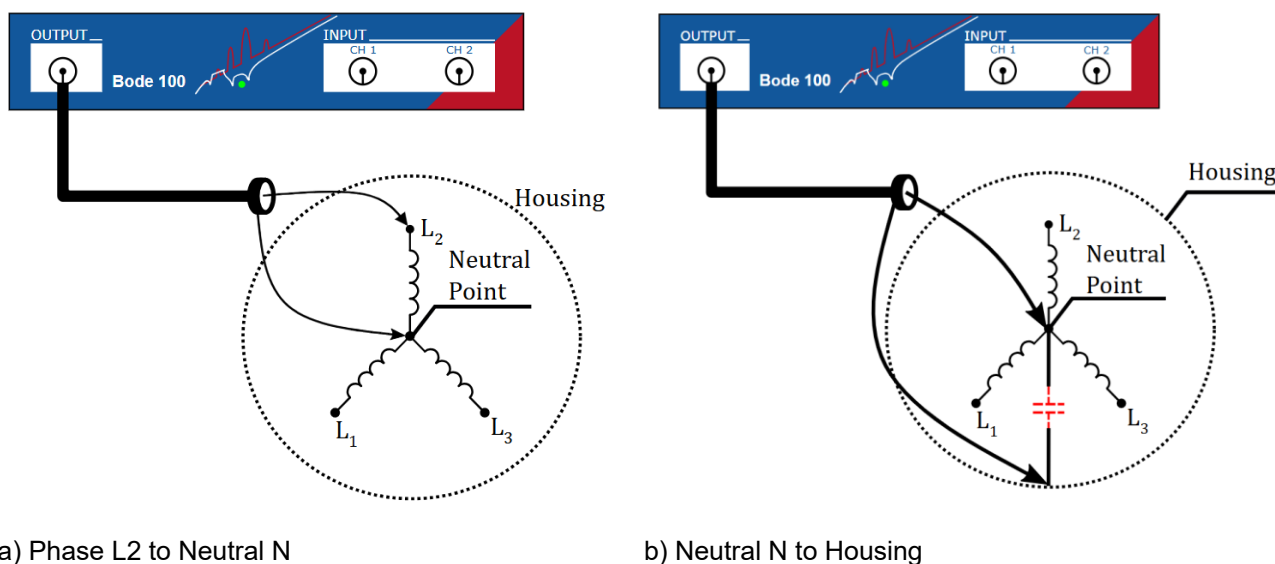


Figure 1: Different impedances of a three-phase motor in star configuration.

3 Measurement Setup

The impedance of the windings in the motor (L1-N, L2-N, L3-N) and the impedance between the neutral point and the housing were measured with the Bode 100 using the One-Port method. The Bode 100 One-Port setup can directly measure impedance/reflection at the output port. It uses the internal 50 Ω source impedance to derive the impedance connected at the output. The DUT must be connected directly to the output as shown in the following figure:

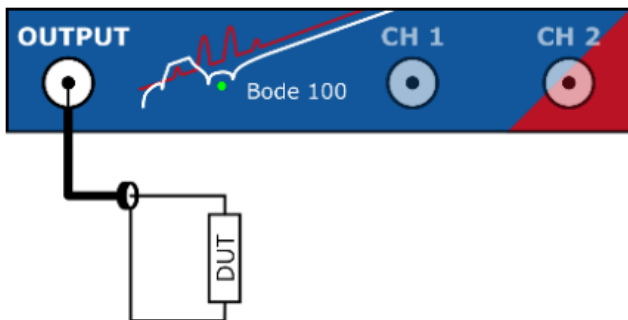


Figure 2: One-Port measurement setup.

The DUT is connected to the Bode 100 housing (GND) via the BNC shield.

The recommended impedance range for this measurement is $\approx 0.5 \Omega$ to 10 k Ω . The Open/Short/Load calibration (preferably performed as User-Range calibration) was used in the measurement.


Please note that the two terminal connections are subject to contact resistance. When using high-quality connectors, the contact resistance can be kept in the low-m Ω range.

3.1 Device Under Test (DUT)

The DUT for the measurement was a three-phase motor with a star-winding configuration. The motor's terminal box facilitates the DUT's measurement process.



a) Overview

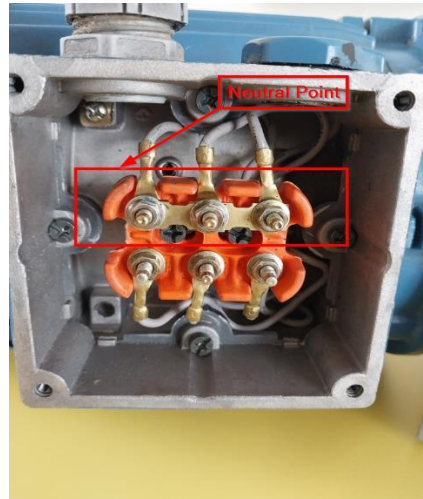

b) Terminal box

Figure 3: Three-phase motor DUT

3.2 DUT Connection

At one end, a 50 Ω coaxial cable is connected to the output of the Bode 100, with a BNC socket adapter attached at the other end. The signal side is utilized for phase measurements, while the shield side is connected to the neutral point as shown in Figure 4.



a) Connect to the terminal box



b) BNC adapter and clips

Figure 4: DUT connection

3.3 Bode Analyzer Suite (BAS) Setup

The Bode Analyzer Suite (BAS) was set up to measure the frequency range from 10 Hz to 10 MHz to capture relevant impedance curve features of the three-phase motor. Three variables in BAS require adjustment depending on the measurement requirements: source level, number of points per measurement, and receiver bandwidth. Below are the criteria to consider when setting up these variables:


- **Source level:** The source level is the signal power output of the Bode 100. Multiple measurements with the same setup are performed to determine if the measurement results differ from the change in source level. Reduce the source level until the measurement does not change with the source level.
- **Number of Points:** The number of points in the BAS are the points measured at each measurement sweep.
- **Receiver Bandwidth:** Lowering the bandwidth will reduce noise and increase measurement time.

Frequency	Sweep	Fixed
Start frequency	10 Hz	
Stop frequency	10 MHz	
Center	5.000005 MHz	
Span	9.99999 MHz	
Get from zoom		
Sweep	Linear	Logarithmic
Number of points	201	
Level	Constant	Variable
Source level	0 dBm	
Attenuator	Receiver 1	Receiver 2
	10 dB	10 dB
Receiver bandwidth	30 Hz	

Figure 5: BAS settings for Three-phase motor impedance measurement.

3.4 Calibration

Calibrating the measurement setup before conducting any measurements is essential. We recommend performing a User-Range impedance calibration to ensure accurate results. The Open-Short-Load calibration is particularly effective in eliminating parasitic errors of the cable, such as setup inductance and capacitance.

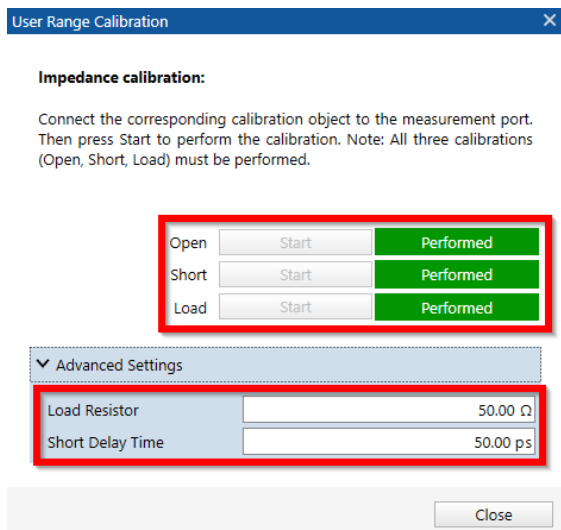

a) Calibration window



b) Open connection



c) Short connection



d) Load connection

Figure 6: Impedance calibration

Note that the BNC to Clip adapter was not included in the calibration. However, the capacitance of the adapter with clips is estimated to be in the single pF region and the inductance will be significantly smaller than the winding inductance. Therefore, it is estimated that the error from the adapter can be ignored.

4 Results

The impedance results for each winding (Figure 7 and Figure 8) show characteristic inductive behavior. As expected, the impedance magnitude is lower at frequencies below 1 kHz. However, at frequencies between 1 kHz and 10 kHz, the magnitude increases considerably, displaying inductive behavior. This indicates that at high frequencies, the motor's windings exhibit greater opposition to the flow of alternating current.

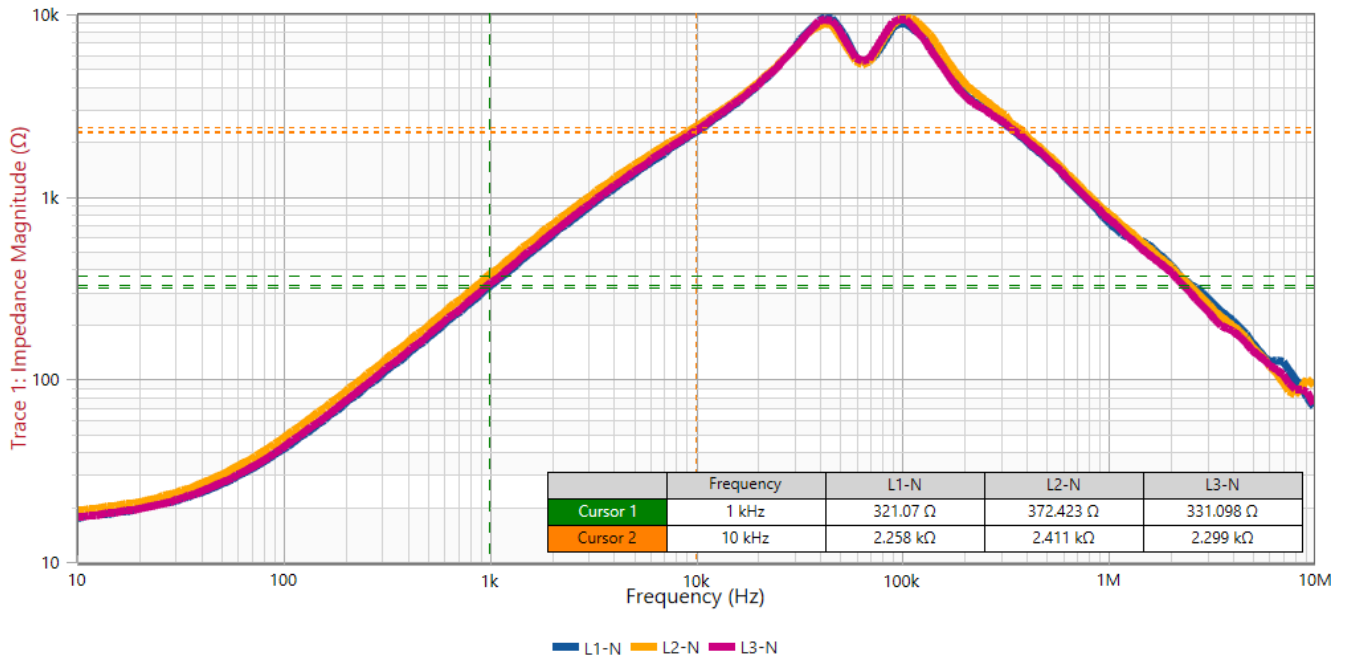


Figure 7 Impedance Magnitude of the motor phases

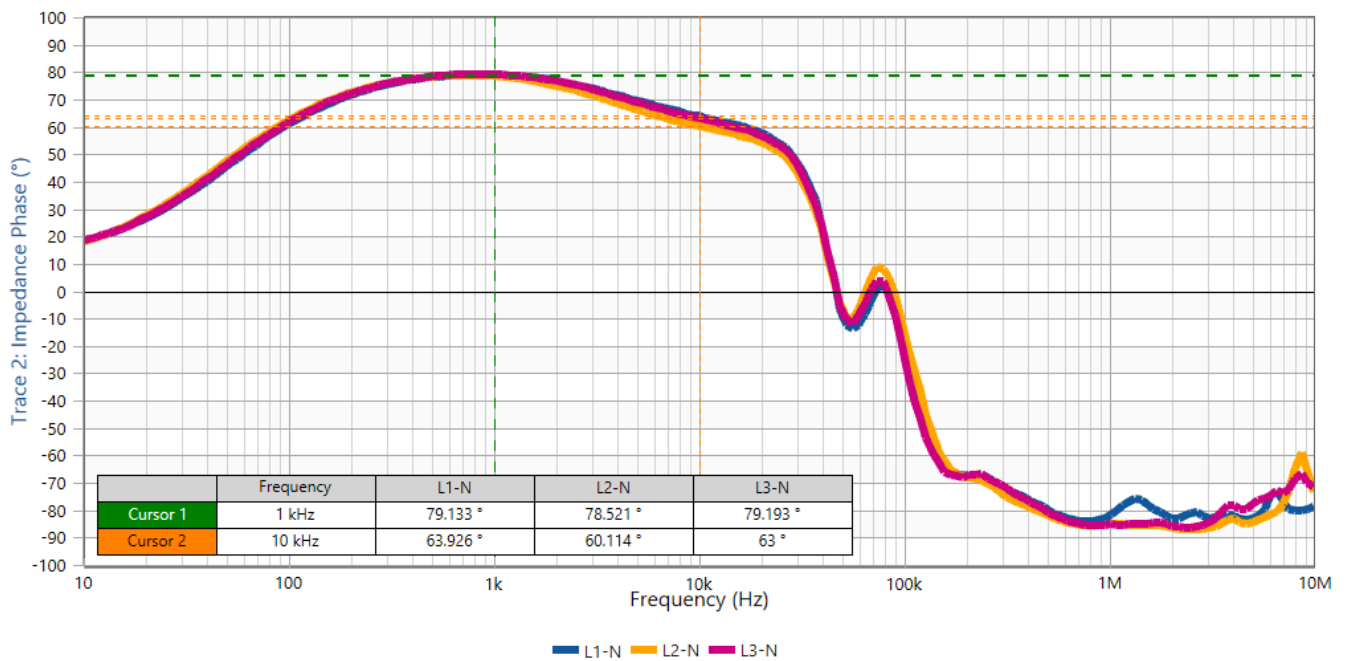


Figure 8 Impedance Phase of the motor phases

At roughly 50 kHz, the impedance shows a resonance frequency and changes from inductive to capacitive behavior because of parasitic capacitance in the winding. Above 100 kHz, the winding shows purely capacitive behavior.

The capacitance between the neutral point and the motor's housing can vary depending on the motor's specific design and construction. Figure 9 shows the impedance measured between the neutral point and motor housing. Up to the resonance frequency of the windings, approximately 55 kHz, a single capacitance predominates in the measurement. As shown in Figure 10, the capacitance is approximately 2.5nF between 5 kHz and 10kHz. Around the resonance frequency, a simple single capacitor cannot model the measured behavior. Figure 10 illustrates that at higher frequencies, around 1 MHz, the capacitance is roughly 0.7nF.

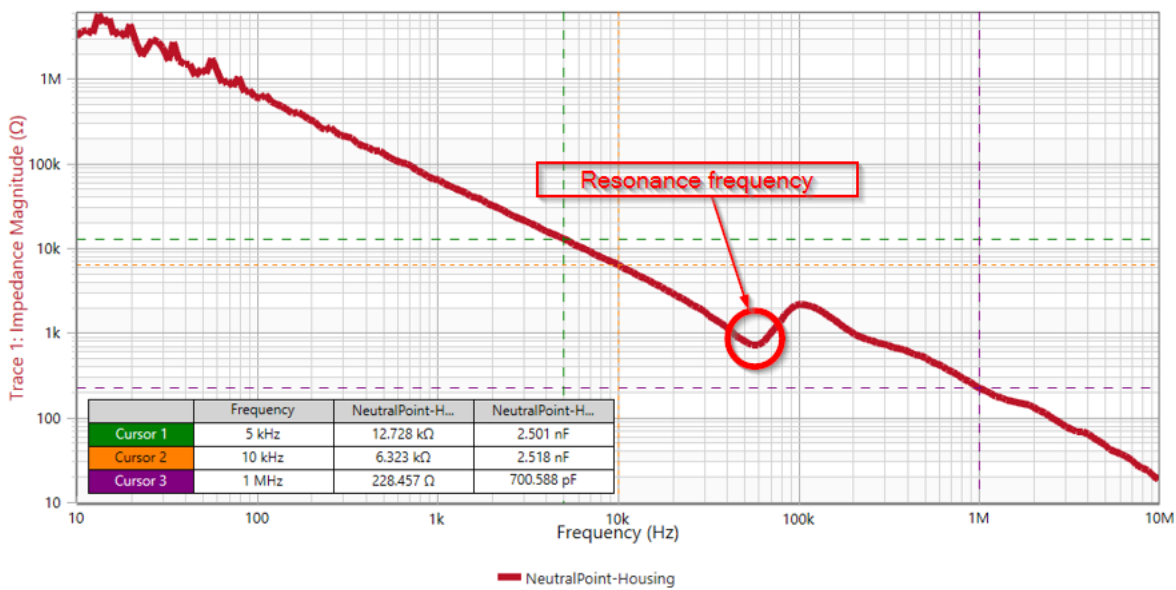


Figure 9 Impedance measurement between neutral point and housing

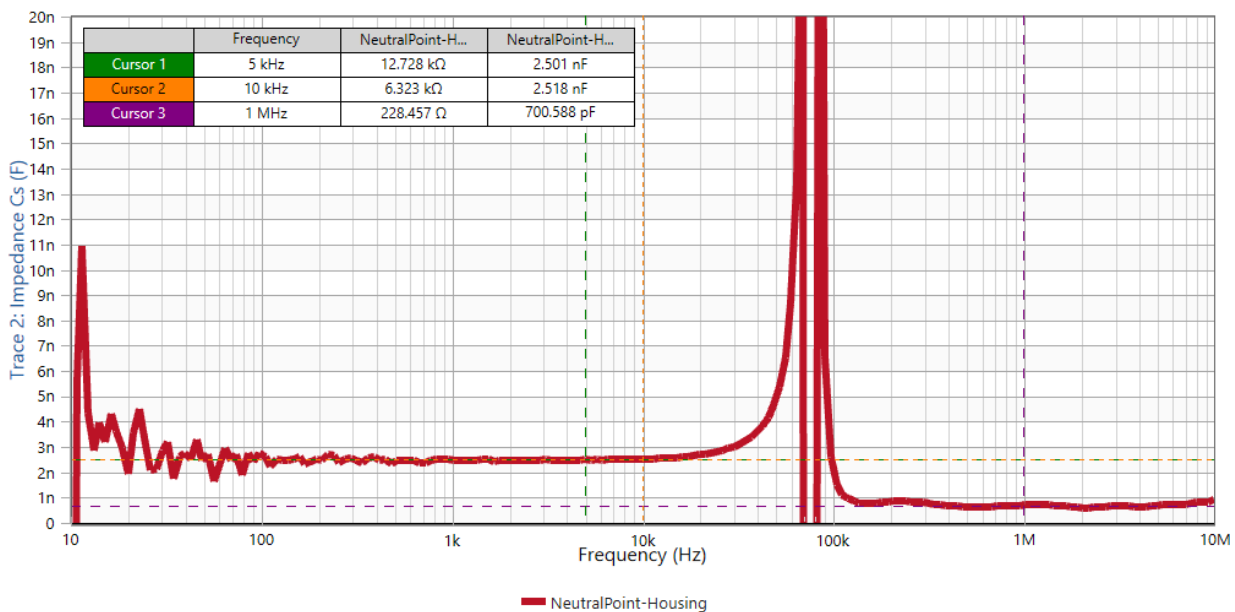


Figure 10 Impedance displayed as equivalent capacitance

5 Conclusion

In this document we have shown that the Bode 100 is perfectly suitable to measure the impedance response of motor windings from 1 Hz up to 50 MHz. A simple One-Port measurement method is suitable for this application. Connection can be made by a simple BNC to 4 mm adapter with crocodile clips. The parasitics of the adapter do not significantly impact the measurement up to several MHz. In summary, we can conclude:

- The insulation capacitance of the motor was measured to be 2.5 nF.
- The resonance frequency of the motor winding was measured to be around 50 kHz.
- The results indicate that the methodology used to determine the impedance of the motor windings is effective and easy to use.



OMICRON Lab is a division of OMICRON electronics GmbH, specialized in providing Smart Measurement Solutions to professionals such as scientists, engineers and teachers engaged in the field of electronics. It simplifies measurement tasks and provides its customers with more time to focus on their real business.

OMICRON Lab was established in 2006 and is meanwhile serving customers in more than 60 countries. Offices in America, Europe, East Asia and an international network of distributors enable a fast and extraordinary customer support.

OMICRON Lab products stand for high quality offered at the best price/value ratio on the market. The products' reliability and ease of use guarantee trouble-free operation. Close customer relationship and more than 30 years in-house experience enable the development of innovative products close to the field.

Europe, Middle East, Africa

OMICRON electronics GmbH

Phone: +43 59495

Fax: +43 59495 9999

Asia Pacific

OMICRON electronics Asia Limited

Phone: +852 3767 5500

Americas

OMICRON electronics Corp. USA

Phone: +1 713 830-4660